


Qualitative test to aid in the diagnosis of COVID-19



## ARISTA<sup>™</sup> COVID-19 Antigen Rapid Test (Nasal Test)

93.3% SENSITIVITY 100% SPECIFICITY



## **OUICKER AND MORE CONVENIENT TESTING** THAN EVER BEFORE.

The ARISTA™ COVID-19 Antigen Rapid Test is a screening tool for selftesting for early Covid-19 detection. Accurate, fast and simple to use with a less invasive sample collection method and get your result within 15 minutes. Able to detect 31 mutated variants including Alpha, Beta, Gamma, Delta etc. Approved by the Medical Device Authority (MDA).

### HIGHLY SCALABLE FOR SAFER SCHOOLS. WORKPLACES, AND OTHER SPACES.

Paired with the Viva Life App, you have the option to securely store all your records on your phone and generate a digital certificate whenever required. It's all in your hands.

## VERIFIABLE DIGITAL TEST CERTIFICATES

## Viva Life Platform

ARISTA Biotech have developed an enterprise solution to facilitate the re-opening of businesses with safer spaces for all.



Individuals can generate and store ready-to-display verifiable digital test certificates via the Viva Life App



Organisations can oversee the test <u>status of their</u> people via the Viva Life Enterprise Account





### **ARISTA Biotech Pte. Ltd.**

## **Onecare Biotech Sdn Bhd**

AUTHORISED Unit S-08-02, 8th floor, First Subang, Jalan SS 15/4G REPRESENTATIVE 47500 Subang Jaya, Selangor Darul Ehsan, Malaysia


### Clotech Sdn Bhd

DISTRIBUTOR No. 24-1, Jalan Medan Setia 2, Damansara 50490 Kuala Lumpur, Wilayah Persekutuan, Malaysia Tel: +603-2011-3666 / +6017-676-7608 Email: salina@drclo.com.my



Qualitative test to aid in the diagnosis of COVID-19

### **TEST KIT CONTENTS**



Test cassette (1x)



Dropper with

protective cap (1x)



Plastic Biohazard Disposal Bag

Instructions for Use (1x)

### HOW TO USE

### 1 - Anterior nasal sample collection.


- A. Remove the sterile swab from the peel-pack being careful to avoid touching the sponge tip with your hands or contacting it with any foreign surface.
- B. Insert the swab sponge tip 1.5cm (3/4 inch) into your nostril.
- C. Slowly rotate the swab in a circular path against the inside of your nostril at least 4 times for a total of 15 seconds.
- D. Using the same swab, repeat steps (B) and (C) in the other nostril.

### 2 – Preparing the sample specimen.

A. Fully immerse the swab sponge tip into the diluent. To ensure all the sample from the swab is mixed into the inserting diluent, rotate the swab stick in a twisting motion in the tube diluent for 30 seconds while squeezing tube against the swab sponge tip.



B. Continue to squeeze the sides of the tube while removing the swab so as to extract all the liquid from the swab sponge tip. Then safely dispose of the swab.




C. Hold the dropper by the protective cap while long-pointed end into the tube until it is securely fitted.



#### 3 - Conducting the test.

- A. Gently mix the sample again by 15-30 rotating the tube for 5 seconds stirring motion. Then remove the remove the protective sap from the dropper.
- B. Remove the test cassette from its foil pack (if you haven't previously done so).

C. Invert the tube and squeeze 3 drops into the smaller rectangular sample well at the bottom of the test cassette (not the larger rectangular C/T results window at the top of the cassette). Note: you may continue the testeven if you inadvertantly applied 4 drops.



D. Start the stopwatch and read the test results after 15 minutes.

Note: after 30 minutes, test results no longer considered valid.



### 4 - Interpreting test result.

#### Negative test result



If the "T" line is blank and the "C" line displays a visable colour band (even if faint) then the result is negative and you are unlikely to have COVID-19.

Note: Negative results are presumptive should not be used as the sole basis for infection control decisions, particularly in the presence of clinical signs and symptoms consistent with COVID-19, or in those who have been in close contact with the virus. In these cases, it is recommended that the test is repeated after 1-2 days. In all cases, a definitive diagnosis must be made by a doctor and local health and safety control measures should always be adhered to.



Positive test result

If both the "T" line and "C" line display visible colour bands (even if faint), then the test result is positive and you most likely are infected with COVID-19.

Note: Positive results require strict adherence to your local public health authority's guidelines for suspected infections - including confirmatory PCR screening at your local hospital or testing station, self-isolation, and reporting to the applicable authorityalways be adhered to. Invalid test result



If the "C" line is blank, then the test result is considered invalid.

Note: Invalid results are represented by a complete absence of a visible "C" line. In this case, carefully read the "Instructions for Use" and repeat the test. If a repeated test result is invalid, then contact your local product supplier.





WWW.VIVALIFE.APP

VIVALIFE Verifiable digital test certificates



# Viva Life Platform

ARISTA Biotech have developed an enterprise solution to facilitate the reopening of businesses with safer spaces for all.



Individuals can generate and store ready-to-display verifiable digital test certificates via the Viva Life App



CLICK TO DISCOVER

Organizations can oversee the test status of their people via the Viva Life Enterprise Account

• Viva Life is compatible with the full range of products from ARISTA Biotech



Available on the App Store

GET IT ON

Google Play

# Viva Life App – Apple App and Google Play Store

-
4
Ο
ø
0

### **Organization ID**

When added, the user's records will automatically be synced to the specific organization's dashboard.


# Step-1

Add certificate




# Step-2 Scan QR code



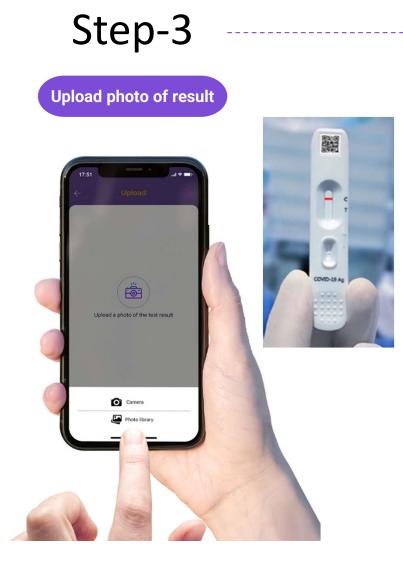


# Step-4


## Confirm date & result

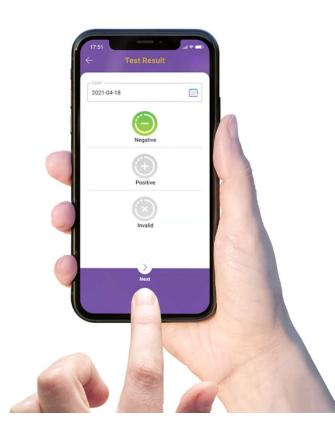

# Step 5

### Preview & save record

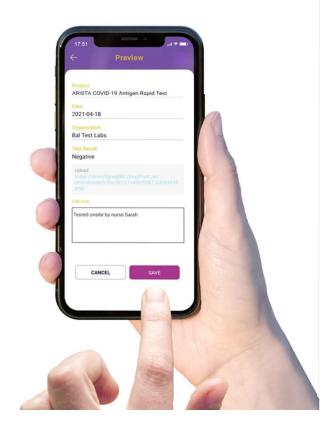




Nucleic Acid Test	2021-04-21
Antibody Test	2021-02-18



# **Success**





View comprehensive test history and delete records

Records	
elect category COVID-19 Antigen Test	•
2021-07-27	Negative
2021-06-23	Invalid •
2021-06-18	Positive
2021-05-27	
2021-04-01	Positive
2021-02-23	Negative >

	ecord Detail
Date	2021-05-27
Product	ARISTA COVID-19 Antigen Rapid Test
Manufacturer	ARISTA Biotech Pte. Ltd.
Organisation	Newco Limited
Serial Number	ANTIGEN TEST0049
Result	Positive
Attachment	1
Note	Test





Viva Life App offers individual users an easy to access Smart Pass to simplify their lives by creating digital test certificates for convenient display.


#### Slide 9


## Viva Life Enterprise Account

Viva Life Enterprise Account is compatible with the Viva Life App and syncs individual users' records to an organization dashboard, enabling the organization to facilitate safer environments for their people.

The enterprise account can integrate one or more organization dashboards where each dashboard can represent a separate branch or department of the enterprise – with login privileges to permit access to different levels of enquiry.



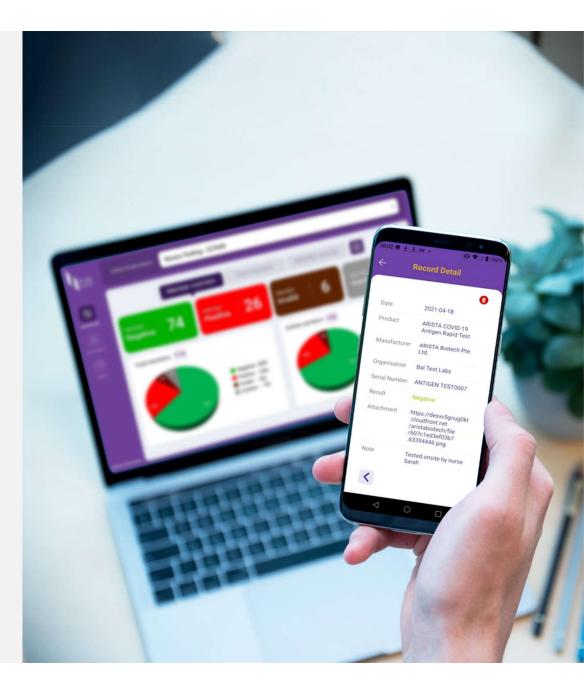

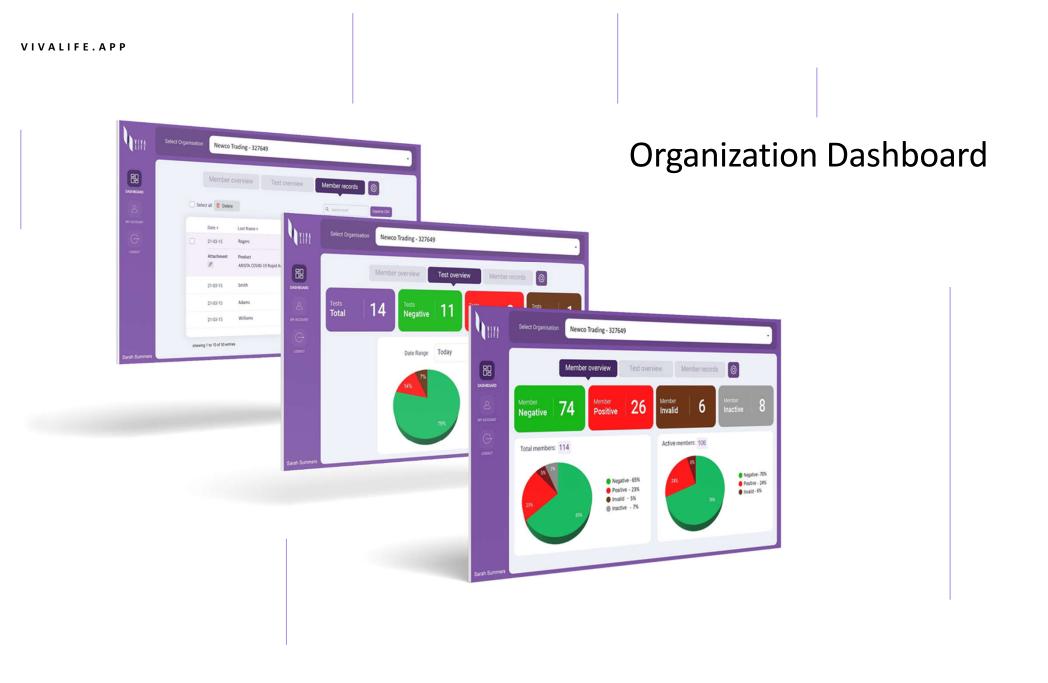


## **Member Overview**

A summary of total members linked to the organization dashboard categorized by:

- Active members: tested in the past 7 days categorized by Negative / Positive / Invalid results
- ii. Inactive members: tested more than 7 days ago


CLICK TO DISCOVER

 $(\cdot)$ 

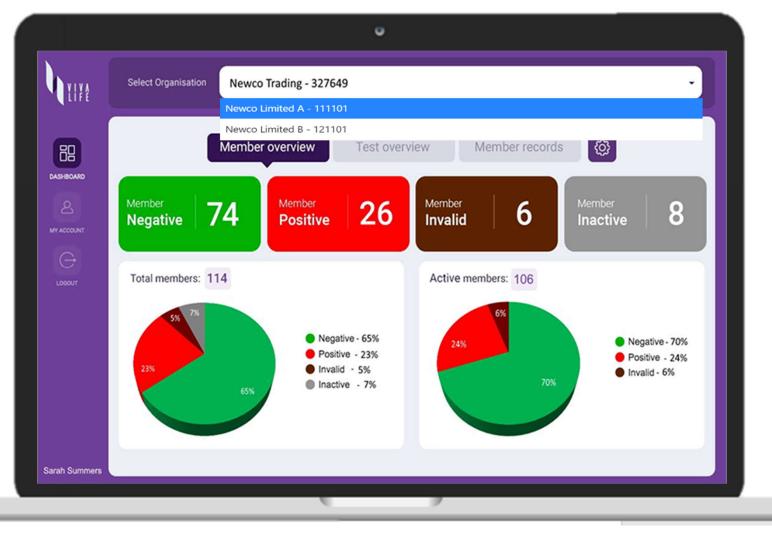

## **Test Overview**

A summary of total tests linked to the organization dashboard categorized by Negative / Positive / Invalid results within a user-selected date range.

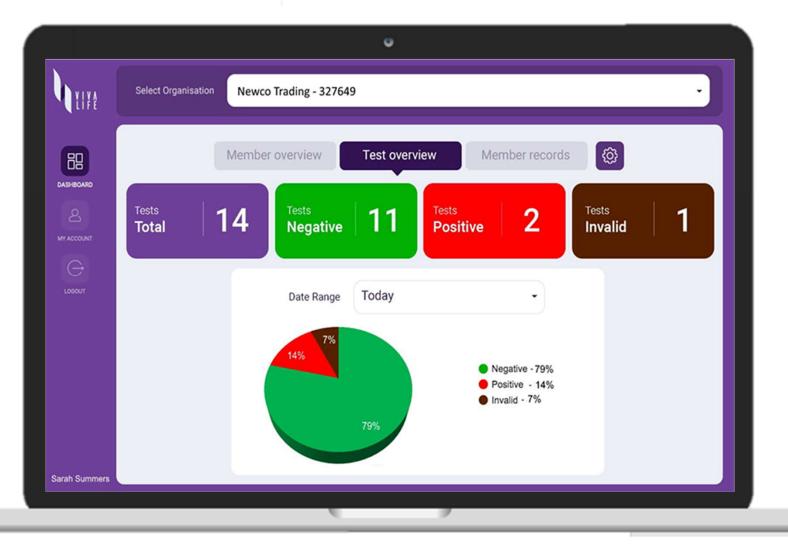

# Member records

Detailed drill-down records of all members linked to the organization dashboard.

¥ê	Select Organisation	Newco T	rading - 327649				
	(	Member o	overview	Test overview	Member rec	cords	
ued	🗌 Sele	ct all 🔋 Delete			Q Search resul	Export to CSV	
NT		Date :	Last Name :	First Name	Category :	Result =	
		21-03-15	Rogers	Barry	Antigen	Positive 👻	
		Attachment	Product ARISTA COVID-19 R	tapid Antigen Test		Serial Number 45367334567	
		21-03-15	Smith	Paul	Antigen	Negative	
		21-03-15	Adams	Mary	Antigen	Invalid	
		21-03-15	Williams	Paula	Antigen	Positive	
mmers	showing	g 1 to 10 of 50 entrie	5		Previo	ous 1 2 3 4 5 Next	

# **Dashboard Settings**

Inviting additional Admin or Overview users to the dashboard - or removing user access to the dashboard

		Ũ	
LIFE			Settings
<u>₹</u>	111101- Newco Limited A		
2	Users		•
	Name	Status	
0	Greg Summers	Owner	
	David Cheung	Admin	<b>立</b>
E	Ailing Pon	Admin	<b>前</b>
	SX	Admin	â
	Lyla Yuan	Admin	â
	Wendy Jacobs 30	Overview	â
Greg Sum			

# Message Center

Invitation notifications and status updates

	v	
LIFE		Message center
 B	Greg Summers has invited you to join the Viva Life dashboard for Newco Limited B a few seconds ago Accept Decline	
2	Graham Murphy has been added as an overview user of Newco Limited A <sup>3</sup> minutes ago	
	Sarah Summers has been added as an overview user of Newco Limited A 4 days ago	
© ©	Raven Annable has been added as a member of Newco Limited A 4 days ago	
Ð	Kevin Williams has been added as a member of Newco Limited A 4 days ago	
	Joseph Stone has been added as a member of Newco Limited A 4 days ago	
	Paula Nichol has been added as a member of Newco Limited A 4 days ago	
	Sam Rockwell has been added as a member of Newco Limited A 4 days ago	
Greg Sum	Show More	



The Viva Life Enterprise Account facilitates the management of the organization's surveillance testing program and provides instant data feedback to enable immediate steps to limit the risk of business shutdown.

DC 159 Viva Life Intro V1.1